

用紙サイズは
A4に設定すること

25 mm

178 mm

原稿の種類
(Paper, Technical Note,
Letter) を書く

Paper

3行あける

2
行分

Analysis of SO₂ Measurement Accuracy by Multiwavelength DIAL

左右中央
に書く

13ポイントまたは18級

Taro Denshi *^{a)} Member,

Hanako Denki ** Non-member

10ポイントまたは13級

左右中央に書く
1行に2名までは横に並べて記入可。
3名以上は改行して記入。

(Manuscript received Jan. 00, 2000, revised May 00, 2000)

16 mm

16 mm

This paper presents two multiwavelength methods to improve the accuracy of a DIAL system for measuring SO₂ in the lower atmosphere: a dual-DIAL method using three or four wavelengths, and a curvefitting method using five wavelengths. By the selection of appropriate wavelengths, these methods can eliminate the effects of ozone and aerosols. Since there is no significant difference in accuracy between the four wavelength dual-DIAL and curvefit methods, the former is advantageous for SO₂ detection in view of the measurement and data processing speeds.

左右
2字
分あける

Keywords : laser radar, SO₂, DIAL, multiwavelength differential absorption

8.5ポイントまたは12級


1行あける

1行あける

2
行分

1. Introduction

LIDAR (LIght Detection And Ranging) has been used for measurement of atmospheric pollutants by Raman scattering, resonant fluorescence, and differential absorption⁽¹⁾. Fig. 1 is a schematic diagram of a LIDAR system. This apparatus transmits laser radiation into the atmosphere, collects light backscattered by atmospheric molecules and particulates using a receiving telescope, and converts it to an electric signal using a photodetector such as a photomultiplier tube. The measurement height is obtained from the time delay between illumination and detection. Therefore, to measure the height profile one measures the received photon counts as a function of time delay relative to illumination using a multichannel scaler. The measurement range resolution ΔR is determined by the time width of the channel $\Delta t = 2\Delta R/c$, where c is the speed of light. The smaller the time Δt , the better the range resolution, but the photon count per channel becomes less and the relative error larger.

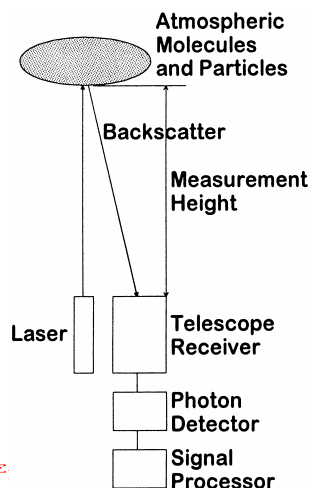

図を入れた
行の余白に
は本文を流
さない

図の説明は左右2字
中央に書く

Fig. 1. Schematic diagram of a LIDAR system.

This paper examines DIAL (Differential Absorption Lidar), a method to obtain the concentration profile of the measurement target molecule from the backscatter intensity at two or more illumination wavelengths. The measurement target is atmospheric SO₂, which is a substance causing acid rain. Until now, measurements of atmospheric SO₂ have been limited mainly to cases of localized SO₂ concentrations, e.g. smokestack exhaust and volcanic eruptions⁽²⁾⁻⁽⁴⁾. In these cases, the SO₂ concentration is over 100 ppb, therefore the measurement was relatively easy and the measurement accuracy was not a problem. However, when measuring SO₂ in the ambient atmosphere, its concentration is of ppb order, and the measurement accuracy becomes an issue. We performed a theoretical analysis of the measurement accuracy of conventional two-wavelength DIAL, and indicated the necessity of eliminating effects due to ozone

and other substances which cause measurement error⁽⁵⁾. In this paper, we examined the measurement accuracy of dual-DIAL methods using three or four wavelengths (consisting of a combination of two two-wavelength DIAL pairs) and a curvefit method using five wavelengths.

2. Multiwavelength Differential Absorption

2.1 Fundamentals of DIAL The received energy for a LIDAR is given by the following LIDAR equation:

$$E_r(R, \lambda_i) = [E_0 \eta A] \frac{\Delta R}{R^2} \beta_x(R) \times \exp \left[-2 \int_0^R (\alpha_0 + \alpha_x) dR' \right]$$

..... (1)

Here $E_r(R, \lambda_i)$ is the backscattered photon energy received from range between R and $R + \Delta R$ from the illumination laser, λ_i the illumination wavelength, E_0 the illumination energy, η the optical efficiency of the

4. Conclusion

In this paper, we calculated the error due to ozone and aerosols in measurement of SO₂ concentrations of ppb order using DIAL. The statistical error of the return signal and background noise can

本文は
9ポイント
または
13級

248 mm (60行)

8.5ポイント
または
12級

This paper is based on "Analysis of SO₂ Measurement Accuracy by Multiwavelength DIAL" published in XXXX Research Report, No.XX (2012-3)

- a) Correspondence to: Taro Denshi. E-mail: taro@denshi.ac.jp
- * Technical Research Labs., Shin-nichi Electric Co., Ltd. 7-2, Gobancho, Chiyoda-ku, Tokyo 102-0076, Japan
- ** Technical Labs., Kagoshima Electron Corp. 2-100, Daikan-cho, Kagoshima 890-0099, Japan

オモ
テキ
ケイ
85ミ
リ

注: 「1字あるいは2字さげる」は、日本語文字の1字分あるいは2字分相当として下さい。

24 mm

2 段通しの表は左右 165 mm 以内
 1 段のときは左右 75 mm 以内

表の説明は左右 2 字分あけ、中央に書く

Table 2. Nominal parameters and rated values of tested DC servo motor.

表中は
7 ポイント
または 10 級

rated output	0.8 kW	K_t	0.48 N·m/A
rated current	11 A	L	1.8 mH
rated speed	1,750 rpm	R	0.66 Ω
K_e	0.48 V·s/rad	J	9.8×10^{-3} kg·m ²

↑ 1 行あける

be overcome by improving the system constant (laser output, receiver area, optical efficiency of the receiver). On the other hand, systematic errors due to ozone and erosols are inherent in the measurement method, and cannot be eliminated solely by improving the system constant. In conentional two-wavelength DIAL, the systematic error is over 1.5 ppb and the measurement accuracy is insufficient. In order to improve the measurement accuracy, a multiwavelength differential absorption method using three or more wavelengths is effective. In this paper we have considered dual-DIAL methods using three or four wavelengths and a curvefit method using five wavelengths, and indicated that the measurement errors due to ozone and aerosols can be reduced relative to conventional DIAL or eliminated. When these methods are compared, four-wavelength dual-DIAL is superior in view of measurement accuracy and measurement/processing speeds.

Acknowledgement

This research was supported by aaaa.


References

- (1) E. D. Hinkley, ed. : Laser Monitoring of the Atmosphere, Springer-verlag, Berlin (1976)
- (2) H. Edner, K. Fredriksson, A. Sunesson, S. Svanberg, L. Unéus, and W. Wendt : "Mobile remote sensing system for atmospheric monitoring", *Appl. Opt.*, Vol.26, pp.4330-4335 (1987)

- (3) H. Edner, P. Ragnarson, S. Svanberg, E. Wallinder, R. Ferrara, R. Cioni, B. Raco, and G. Taddeucci : "Total fluxes of sulfur dioxide from the Italian volcanoes Etna, Stromboli, and Vulcano measured by differential absorption lidar and passive differential optical absorption spectroscopy", *J. Geophys. Res.*, Vol.99, pp.1820-1825 (1994)
- (4) K. Fredriksson, B. Galle, K. Nyström, and S. Svanberg : "Lidar system applied in atmospheric pollution monitoring", *Appl. Opt.*, Vol.18, 2998-2302 (1979)
- (5) N. Goto : "SO₂ measurement by laser radar", Denki University Research Report No.95085 (1995)
- (6) J. D. Klett : "Stable analytical inversion solution for processing lidar returns", *Appl. Opt.*, Vol.20, pp.211-215 (1981)

ボード

Taro Denshi



(Member) He received a Ph.D. degree in physics from Denshi Institute of Technology in 1995, and is presently an assistant engineer at Shin-nichi Electric Co., Ltd. He has worked on laser spectroscopy, and development of LIDAR systems. Japan Applied Physics Society, American Physical Society member.

↑ 1 行あける

Hanako Denki



(Non-member) She received a Ph.D. degree in electrical engineering from Electric University in 1984, and is presently a Chief engineer at Kagoshima Electron Corp. She has worked on analysis of electromagnetic flow coupler pumps, development of Cherenkov radiation monitors for nuclear inspection, and development of laser beam intensity transformation techniques. Japan Applied

Physics Society, Laser Society of Japan, Optical Society of America member.

付録を付ける場合は、文献の後、著者紹介の前に挿入する。

謝辞を記載する場合は、本文の最後、文献の前に挿入する。