

# Analysis of SO<sub>2</sub> Measurement Accuracy by Multiwavelength DIAL

Taro Denshi\*<sup>a)</sup> Member, Hanako Denki\*\* Non-member

(Manuscript received Jan. 00, 2000, revised May 00, 2000)

This paper presents two multiwavelength methods to improve the accuracy of a DIAL system for measuring SO<sub>2</sub> in the lower atmosphere: a dual-DIAL method using three or four wavelengths, and a curvefitting method using five wavelengths. By the selection of appropriate wavelengths, these methods can eliminate the effects of ozone and aerosols. Since there is no significant difference in accuracy between the four wavelength dual-DIAL and curvefit methods, the former is advantageous for SO<sub>2</sub> detection in view of the measurement and data processing speeds.

**Keywords** : laser radar, SO<sub>2</sub>, DIAL, multiwavelength differential absorption

## 1. Introduction

LIDAR (LIght Detection And Ranging) has been used for measurement of atmospheric pollutants by Raman scattering, resonant fluorescence, and differential absorption<sup>(1)</sup>. Fig. 1 is a schematic diagram of a LIDAR system. This apparatus transmits laser radiation into the atmosphere, collects light backscattered by atmospheric molecules and particulates using a receiving telescope, and converts it to an electric signal using a photodetector such as a photomultiplier tube. The measurement height is obtained from the time delay between illumination and detection. Therefore, to measure the height profile one measures the received photon counts as a function of time delay relative to illumination using a multichannel scaler. The measurement range resolution  $\Delta R$  is determined by the time width of the channel  $\Delta t=2\Delta R/c$ , where  $c$  is the speed of light. The smaller the time  $\Delta t$ , the better the range resolution, but the photon count per channel becomes less and the relative error larger.

This paper examines DIAL (Differential Absorption Lidar), a method to obtain the concentration profile of the measurement target molecule from the backscatter intensity at two or more illumination wavelengths. The measurement target is atmospheric SO<sub>2</sub>, which is a substance causing acid rain. Until now, measurements of atmospheric SO<sub>2</sub> have been limited mainly to cases of localized SO<sub>2</sub> concentrations, e.g. smokestack exhaust and volcanic eruptions<sup>(2)-(4)</sup>. In these cases, the SO<sub>2</sub> concentration is over 100 ppb, therefore the measurement was relatively easy and the measurement accuracy was not a problem. However, when measuring SO<sub>2</sub> in the ambient atmosphere, its concentration is of ppb order, and the measurement accuracy becomes an issue. We performed a theoretical analysis of the measurement accuracy of conventional two-wavelength DIAL,

This paper is based on "Analysis of SO<sub>2</sub> Measurement Accuracy by Multiwavelength DIAL" published in XXXX Research Report, No.XX (2012)

This paper is based on Reference (1), which published in the International Conference ○○○○ (2020) ©2020 IEEJ.

- a) Correspondence to: Taro Denshi. E-mail: taro@denshi.ac.jp
- \* Technical Research Labs., Shin-nichi Electric Co., Ltd. 7-2, Gobancho, Chiyoda-ku, Tokyo 102-0076, Japan
- \*\* Technical Labs., Kagoshima Electron Corp. 2-100, Daikan-cho, Kagoshima 890-0099, Japan

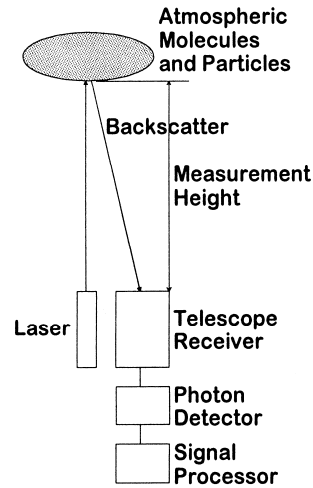


Fig. 1. Schematic diagram of a LIDAR system

and other substances which cause measurement error<sup>(5)</sup>. In this paper, we examined the measurement accuracy of dual-DIAL methods using three or four wavelengths (consisting of a combination of two two-wavelength DIAL pairs) and a curvefit method using five wavelengths.

## 2. Multiwavelength Differential Absorption

**2.1 Fundamentals of DIAL** The received energy for a LIDAR is given by the following LIDAR equation:

$$E_r(R, \lambda_i) = [E_0 \eta A] \frac{\Delta R}{R^2} \beta_x(R) \times \exp \left[ -2 \int_0^R (\alpha_0 + \alpha_x) dR' \right]$$

..... (1)

Here  $E_r(R, \lambda_i)$  is the backscattered photon energy received from range between  $R$  and  $R+\Delta R$  from the illumination laser,  $\lambda_i$  the illumination wavelength,  $E_0$  the illumination energy,  $\eta$  the optical efficiency of the

## 4. Conclusion

In this paper, we calculated the error due to ozone and aerosols in measurement of SO<sub>2</sub> concentrations of ppb order using DIAL. The statistical error of the return signal and background noise can

Use doubleline  
16 mm  
Use 2 lines for the heading  
Use 9 pt font  
248 mm (60 lines)

Center the title  
Triple Space  
Double Space  
Double Space  
Double Space  
16 mm  
Indent two strokes each on both margins

Do not fill the blank space around the figures with text  
Use 7 pt font in a figure

8 mm between the columns

9 pt  
Center the caption  
Double Space

Two strokes space after the heading

[An equation starts at two-stroke indent]

8.5 pt

24 mm

Table should be prepared to fit one-column; within 75 mm, or two-column; within 165 mm

Table 2. Nominal parameters and rated values of tested DC servo motor

rated output	0.8 kW	$K_t$	0.48 N·m/A
rated current	11 A	$L$	1.8 mH
rated speed	1,750 rpm	$R$	0.66 $\Omega$
$K_e$	0.48 V·s/rad	$J$	$9.8 \times 10^{-3}$ kg·m <sup>2</sup>

Use 7 pt font in a table

Double Space

be overcome by improving the system constant (laser output, receiver area, optical efficiency of the receiver). On the other hand, systematic errors due to ozone and aerosols are inherent in the measurement method, and cannot be eliminated solely by improving the system constant. In conventional two-wavelength DIAL, the systematic error is over 1.5 ppb and the measurement accuracy is insufficient. In order to improve the measurement accuracy, a multiwavelength differential absorption method using three or more wavelengths is effective. In this paper we have considered dual-DIAL methods using three or four wavelengths and a curvefit method using five wavelengths, and indicated that the measurement errors due to ozone and aerosols can be reduced relative to conventional DIAL or eliminated. When these methods are compared, four-wavelength dual-DIAL is superior in view of measurement accuracy and measurement/processing speeds.

**Acknowledgement**


This research was supported by aaaa.

**References**


(1) E. D. Hinkley, ed. : Laser Monitoring of the Atmosphere, Springer-verlag, Berlin (1976)  
 (2) H. Edner, K. Fredriksson, A. Sunesson, S. Svanberg, L. Unéus, and W. Wendt : "Mobile remote sensing system for atmospheric monitoring", *Appl. Opt.*, Vol.26, pp.4330-4335 (1987)

(3) H. Edner, P. Ragnarson, S. Svanberg, E. Wallinder, R. Ferrara, R. Cioni, B. Raco, and G. Taddeucci : "Total fluxes of sulfur dioxide from the Italian volcanoes Etna, Stromboli, and Vulcano measured by differential absorption lidar and passive differential optical absorption spectroscopy", *J. Geophys. Res.*, Vol.99, pp.1820-1825 (1994)  
 (4) K. Fredriksson, B. Galle, K. Nyström, and S. Svanberg : "Lidar system applied in atmospheric pollution monitoring", *Appl. Opt.*, Vol.18, 2998-2302 (1979)  
 (5) N. Goto : "SO<sub>2</sub> measurement by laser radar", Denki University Research Report No.95085 (1995)  
 (6) J. D. Klett : "Stable analytical inversion solution for processing lidar returns", *Appl. Opt.*, Vol.20, pp.211-215 (1981)

Use boldface



**Hanako Denki**



(Member) He received a Ph.D. degree in physics from Denshi Institute of Technology in 1995, and is presently an assistant engineer at Shin-nichi Electric Co., Ltd. He has worked on laser spectroscopy, and development of LIDAR systems. Japan Applied Physics Society, American Physical Society member.

Double Space

(Non-member) She received a Ph.D. degree in electrical engineering from Electric University in 1984, and is presently a Chief engineer at Kagoshima Electron Corp. She has worked on analysis of electromagnetic flow coupler pumps, development of Cherenkov radiation monitors for nuclear inspection, and development of laser beam intensity transformation techniques. Japan Applied Physics Society, Laser Society of Japan, Optical Society of America member.